

Operating and Service Manual Modification

**Agilent Technologies
85320A/B H20
Mixer Modules
0.1 to 3 GHz**

**Use this modification with manual part number
85320-90001.**



Part Number: 85320-90032

Printed in USA

July 23, 1996

Revision 2.2

© Copyright 1996 Agilent Technologies, Inc.

Notice.

The information contained in this document is subject to change without notice.

Agilent Technologies makes no warranty of any kind with regard to this material, including but not limited to, the implied warranties of merchantability and fitness for a particular purpose. Agilent shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Restricted Rights Legend

Use, duplication, or disclosure by the U.S. Government is subject to restrictions as set forth in subparagraph (c)(1)(ii) of the Technical Data and Computer Software clause at DFARS 252.227-7013 for DOD agencies, and subparagraphs (c)(1) and (c)(2) of the Commercial Computer Software Restricted Rights clause at FAR 52.227-19 for other agencies.

Hewlett-Packard to Agilent Technologies Transition

This documentation supports a product that previously shipped under the Hewlett-Packard company brand name. The brand name has now been changed to Agilent Technologies. The two products are functionally identical, only our name has changed. The document still includes references to Hewlett-Packard products, some of which have been transitioned to Agilent Technologies.

Warranty

Certification

Hewlett-Packard Company certifies that this product met its published specifications at the time of shipment from the factory. Hewlett-Packard further certifies that its calibration measurements are traceable to the United States National Institute of Standards and Technology (NIST, formerly NBS), to the extent allowed by the Institute's calibration facility, and to the calibration facilities of other International Standards Organization members.

Warranty

This Hewlett-Packard system product is warranted against defects in materials and workmanship for a period corresponding to the individual warranty periods of its component products. Instruments are warranted for a period of one year. During the warranty period, Hewlett-Packard Company will, at its option, either repair or replace products which prove to be defective.

Warranty service for products installed by HP and certain other products designated by HP will be performed at Buyer's facility at no charge within HP service travel areas. Outside HP service travel areas, warranty service will be performed at Buyer's facility only upon HP's prior agreement and Buyer shall pay HP's round trip travel expenses. In all other areas, products must be returned to a service facility designated by HP.

For products returned to HP for warranty service, Buyer shall prepay shipping charges to HP and HP shall pay shipping charges to return the product to Buyer. However, Buyer shall pay all shipping charges, duties, and taxes for products returned to HP from another country.

HP warrants that its software and firmware designated by HP for use with an instrument will execute its programming instructions when properly installed on that instrument. HP does not warrant that the operation of the instrument, or software, or firmware will be uninterrupted or error free.

LIMITATION OF WARRANTY. The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by Buyer, Buyer-supplied software or interfacing, unauthorized modification or misuse, operation outside of the environmental specifications for the product, or improper site preparation or maintenance.

NO OTHER WARRANTY IS EXPRESSED OR IMPLIED. HP SPECIFICALLY DISCLAIMS THE IMPLIED WARRANTIES OR MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.

EXCLUSIVE REMEDIES

THE REMEDIES PROVIDED HEREIN ARE BUYER'S SOLE AND EXCLUSIVE REMEDIES. HP SHALL NOT BE LIABLE FOR ANY DIRECT, INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES, WHETHER BASED ON CONTRACT, TORT, OR ANY OTHER LEGAL THEORY.

Assistance

Product maintenance agreements and other customer assistance agreements are available for Hewlett-Packard products.

For assistance, call your local Hewlett-Packard Sales and Service Office (refer to the listing on the following page).

Servicing

By internet, phone, or fax, get assistance with all your test and measurement needs.

Contacting Agilent

Online assistance: www.agilent.com/find/assist

United States
(tel) 1 800 452 4844

Latin America
(tel) (305) 269 7500
(fax) (305) 269 7599

Canada
(tel) 1 877 894 4414
(fax) (905) 282-6495

Europe
(tel) (+31) 20 547 2323
(fax) (+31) 20 547 2390

New Zealand
(tel) 0 800 738 378
(fax) (+64) 4 495 8950

Japan
(tel) (+81) 426 56 7832
(fax) (+81) 426 56 7840

Australia
(tel) 1 800 629 485
(fax) (+61) 3 9210 5947

Asia Call Center Numbers

Country	Phone Number	Fax Number
Singapore	1-800-375-8100	(65) 836-0252
Malaysia	1-800-828-848	1-800-801664
Philippines	(632) 8426802 1-800-16510170 (PLDT Subscriber Only)	(632) 8426809 1-800-16510288 (PLDT Subscriber Only)
Thailand	(088) 226-008 (outside Bangkok) (662) 661-3999 (within Bangkok)	(66) 1-661-3714
Hong Kong	800-930-871	(852) 2506 9233
Taiwan	0800-047-866	(886) 2 25456723
People's Republic of China	800-810-0189 (preferred) 10800-650-0021	10800-650-0121
India	1-600-11-2929	000-800-650-1101

Safety Considerations

General

Review this product and related documentation to familiarize yourself with safety markings and instructions before you operate the instrument. This product has been designed and tested in accordance with international standards.

Safety Symbols

WARNING

The **WARNING** notice denotes a hazard. It calls attention to a procedure, practice, or the like, that, if not correctly performed or adhered to, could result in personal injury. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

CAUTION

The **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like, which, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.



The product will be marked with this instruction manual symbol when it is necessary for you to refer to the instruction manual.



Indicates hazardous voltages.



Indicates earth (ground) terminal.

Safety Earth Ground

This is a Safety Class I product (provided with a protective earthing terminal). An uninterruptible safety earth ground must be provided from the main power source to the product input wiring terminals, power cord, or supplied power cord set. Whenever it is likely that the protection has been impaired, the product must be made inoperative and secured against any unintended operation.

Before Applying Power

Verify that the product is configured to match the available main power source as described in the input power configuration instructions in this manual.

If this product is to be powered by autotransformer, make sure the common terminal is connected to the neutral (grounded) side of the AC power supply.

Contents

Description	2
Accessories	2
Specifications	3
HP 85310A System Performance Notes	5
Avoiding the Effects of Spurs	7
Calculating Potential Spurs	8
Figure 1: <i>Spur Level Performance in Low Band</i>	
Figure 2: <i>Mechanical Mounting Information</i>	

Description

This manual modification describes the differences in the HP 85320A H20 and HP 85320B H20 compared to the standard HP 85320A and HP 85320B.

The HP 85320A H20 and the HP 85320B H20 are identical in function to the standard HP 85320A and HP 85320B except that the frequency range of operation is 0.1 to 3.0 GHz instead of 2.0 to 26.5 GHz. Fundamental mixing is the only mode of operation.

The HP 85320A H20 test mixer and the HP 85320B H20 reference mixer are designed for use with the HP 85309A H20 and H21 LO/IF distribution units.

Accessories

HP 85320A/B H20 Mixer Modules	
Operating and Service Manual Modification (1)	85320-90032
RF adapter, Type-N (m)/(m), (1) for each module	1250-1475
Mounting bolts, (4) for each module	2940-0287

Specifications

Operating Frequency Range:

0.1 to 3.0 GHz (fundamental mixing mode ONLY)

Maximum Input Levels:

Maximum RF level at RF and LO inputs (damage level): +20 dBm

Table 1-1. Minimum LO Input Levels under Normal Operations

LO Frequency	Minimum Power	Typical Power	Maximum Power
0.1 - 3 GHz	+ 8 dBm	+ 10 dBm	+ 16 dBm

Table 1-2. Conversion Loss (LO at +10 dBm)

LO Frequency	LO Harmonic	Typical Loss	Maximum Loss
0.1 - 3 GHz	1	-12 dB	-16 dB

Connector Types:

Type-N female (all ports)

Weight (approximate):

HP 85320A H20: 0.70 Kg (1.52 lb)

HP 85320B H20: 1 kg (2.2 lb)

Dimensions (excluding connectors):

HP 85320A H20: width = 97 mm (3.8 in)
length = 122 mm (4.8 in)

height = 34 mm (1.3 in)

HP 85320B H20: width = 97 mm (3.8 in)
length = 186 mm (7.3 in)

height = 31 mm (1.2 in)

Rebuilt/Exchange Parts:

This program does not apply to the HP 85320A/B H20

Mechanical mounting information can be found on the last page of this document.

85310A System Performance Notes

HP 85320A/B H20 Mixers and the HP 85309A H2x

The HP 85320A/B H20 mixer modules were designed to be used with HP 85309A H20 and H21 LO/IF distribution units. This combination of products will provide full HP 85320A/B H20 frequency range of operation.

The frequency range of operation consists of two bands: low band operating from 0.1 to 1.0 GHz and high band operating from 0.3 to 3.0 GHz.

HP 85320A/B H20 Mixers and the Standard HP 85309A

If the HP 85320A/B H20 mixer modules are used with a standard HP 85309A, the frequency range of operation is limited to 0.3 to 3 GHz.

HP 85320A/B-H20 Mixer System Performance Note

System performance data — when the HP 85309A H20, -H21, HP 85320A H20, HP 85320B H20, and HP 8510/8530 are combined in a system—is shown in Table 2.

Refer to "Table 5-3" in the "General Information" section of the HP 85310A Operating and Service Manual (85310-90001) when using Table 2.

Table 2. HP 85310A System Performance Data with the HP 85320A/B H20 Mixer		
	0.1 to 0.5 GHz	0.5 to 3.0 GHz
Sensitivity (S/N=1, 0 averages)	-100 dBm	-113 dBm
Compression Level (at 0.1 dB)	-24 dBm	-24 dBm
Dynamic Range	76 dB	89 dB
Crosstalk	90 dB	100 dB
Minimum Phase Lock Power	-55 dBm	-55 dBm
RF Port Match	8 dB	8 dB
Conversion Gain (± 2 dB)	10 dB	10 dB

Definitions:

Sensitivity: The calculated difference between IF noise and RF-IF conversion gain or loss. Averaging will improve sensitivity by $10 \log$ (averaging factor).

Compression level: The point where an RF input level and IF output level are no longer relatively linear within 0.1 dB.

Dynamic range: The calculated difference between compression and sensitivity.

Crosstalk: The coherent RF leakage from the reference channel to the test channel with 1024 averages.

Minimum Phase Lock Power: This term refers to systems using an HP 8350 LO source. Minimum phase lock power is the minimum RF power needed going into the reference mixer to achieve phase lock. *This does not apply to systems with a synthesized LO source.*

Avoiding the Effects of Spurs

The spurious signal levels seen on the HP 8510/30 from the LO source are dependent on the LO power level setting. When using an HP 8360 series synthesized sweeper as the LO source, it is recommended that you set the output power level to +10 dBm. This will minimize potential HP 85310A system spurious signals generated by the HP 8360A source when it is in low band (< 2.0 GHz). With the recommended +10 dBm setting, spur levels may be no greater than -100 dBm. With a power level of +25 dBm you may detect spurs as high as -60 dBm.

In normal HP 8510/30 operation, there are sixteen frequencies that should be avoided due to potential spurs. These frequencies are listed in Table 3. The spurs can be avoided or removed by a number of techniques, such as:

- changing the start or stop frequency by as little as 5 KHz
- using frequency list mode to avoid potential spur frequencies
- changing the multiple source equations on the HP 8510/30 to move the spur to a new frequency
- additionally reducing the LO source power to yield a 4 dB improvement per dB of source power change (Lowering the source power will result in an increase in the noise floor of the measurement system which is not recommended.)

Calculating Potential Spurs

1. Determine if any frequencies of interest are potential spur frequencies. Note that spurs only exist for frequencies < 2.0 GHz.

The mixing spurs have an "order" (M,N) associated with them which determines the mixing products used in their generation. As a rule, orders greater than (12,12) can be ignored. The equations used to predict if a spur problem exists are:

High Side LO

A potential problem if the spur is less than 10 KHz.

$$\left| F - \left(\frac{5.4 \times 10^9 \times (M-N) - 20 \times 10^6}{1-M} \right) + 20 \times 10^6 \right|$$

Low Side LO

A potential problem if the spur is less than 10 KHz. Where (M,N) are ... -3, -2, -1, 1, 2, 3 ... and F is the frequency of interest in MHz.

$$\left| F - \left(\frac{5.4 \times 10^9 \times (M-N) + 20 \times 10^6}{1-M} \right) - 20 \times 10^6 \right|$$

2. Determine the impact on measurement.

If a frequency of interest has a potential spur, its impact should be assessed. The closer equation a.) or b.) is to zero, the larger the spur impact. Figure 1 may be used to approximate the level of the spur.

3. Decide how to minimize spur impact.

The spurs can be avoided or removed by a number of techniques. See "Avoiding the Effects of Spurs" on the previous page.


The top sixteen potential spur frequencies are listed in Table 3.

Table 3. Potential Spurs

Spur Order (M,N)	Normal	8530A Operation
	High Side Frequency (MHz) Source 2:1 (Freq. + 0.02) GHz	Low Side Frequency (MHz) Source 2:1 (Freq. - 0.02) GHz
(-2,-3)	1786.67	1813.33
(7,9)	1776.67	1823.33
(4,5)	1773.33	1826.67
(9,11)	1327.50	1372.50
(5,6)	1325.00	1375.00
(-4,-5)	1064.00	1096.00
(6,7)	1056.00	1104.00
(-5,-6)	883.33	916.67
(7,8)	876.67	923.33
(-6,-7)	754.29	788.57
(8,9)	748.57	794.29
(-7,-8)	657.50	692.50
(9,10)	652.50	697.50
(-8,-9)	582.22	617.78
(10,11)	577.78	622.22
(-10,-11)	472.73	509.09


Notes

1. No spurs will be seen for $F > 2.0$ GHz.
 2. This list is not all encompassing. It is only a list of sixteen frequencies which may cause problems.
 3. Figure 1 may be used to assess the magnitude of the problem.
-

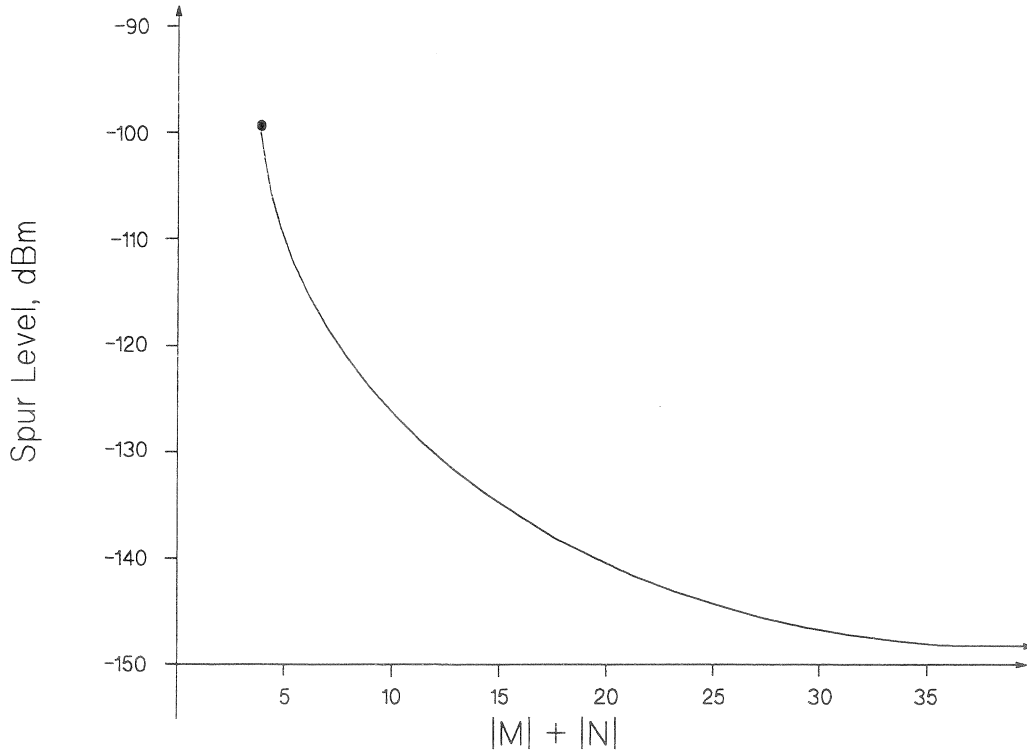

Typical: 85309A Low band spur performance at +10 LO power
 Expect a 4 dB/dB improvement with LO power

Figure 1. Spur Level Performance in Low Band

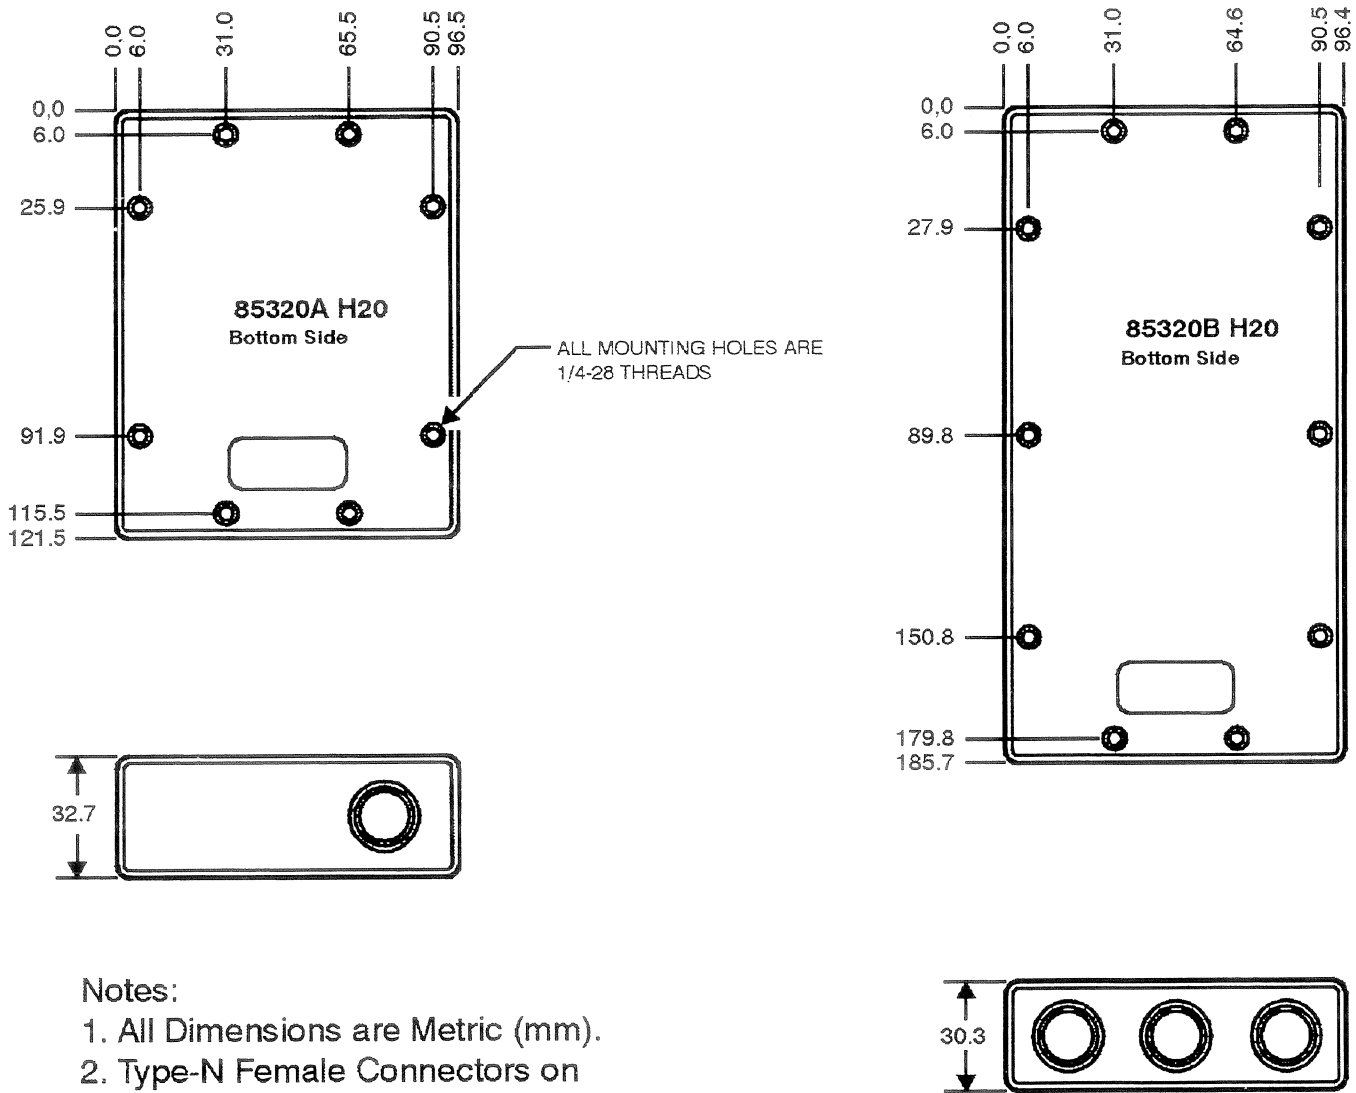

85320A H20
muntinfo.cdr
Rev. 1.0
7/9/96

Figure 2. Mechanical Mounting Information

** For Agilent Internal Reference Only

Customer Order Number

Manufacturing Part Number

85320-90032



Printed in USA

July_23 1996